

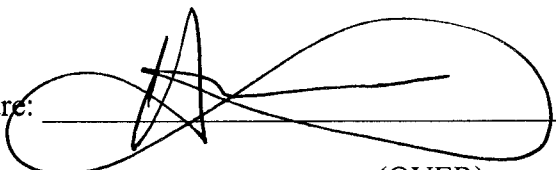
# VERIFICATION OF CALIBRATION REPORT

Of DataMaster cdm Breath test Instrument

State of Alaska

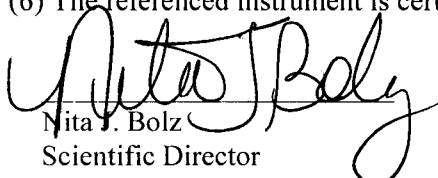
Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program

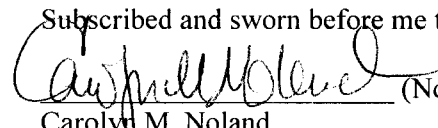
JAN 12 2010


|   |   |
|---|---|
| DataMaster cdm S/N: <u>130193</u>   |   |
| Supervisor/Operator Performing the Verification Procedure:                                    |   |
| Name: <u>JAMES C. GIPSON</u> ID#: <u>4842</u> Date: <u>06 January 10</u>                      |   |
| <b>A</b>  | Agency: <u>Palmer Police Department</u> Phone #: <u>(907) 745-4811</u>      |
|   | Instrument Location: <u>Palmer Police Department</u>                        |
| <b>B</b>  | Alco S/N: <u>77621</u> Target Value: <u>.079</u> High Pressure: <u>1200</u> |
|   | Alco Test Value Average: <u>.080</u> <u>.080</u>                            |
|   | 1 <sup>st</sup> Alco 2 <sup>nd</sup> Alco                                   |
| Signature:  |   |
| (OVER)  |   |

I, Nita J. Bolz, after being first duly sworn, depose and state as follows. (Do Not write in the area below)

- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 20<sup>th</sup> day of January 2010.  
  
(Notary Seal Stamp)  
Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office



# VERIFICATION OF CALIBRATION REPORT

*Of DataMaster cdm Breath test Instrument*

*State of Alaska*

*Scientific Crime Detection Laboratory – Statewide Breath Alcohol Program*

DataMaster cdm S/N: 130193  
130298 (1-12-10 On)

(CONTINUED FROM FRONT PAGE)

**C**

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193 ✓

JANUARY 06, 2010 ✓ C 1/13/10

OPERATOR'S NAME: GIPSON/JAMES/C  
OPERATOR'S NUMBER: 4842  
SUBJECT'S LAST NAME: VERIFICATION OF CAL  
SUBJECT'S FIRST NAME/MI: RJCG0  
O.L. #: 0123456  
DEPT/AGENCY: PLM1  
CASE/REPORT: 01-2345  
TEST TYPE: U  
ALCO TARGET VALUE: .079 ✓  
ALCO S/N: 77621 ✓

### — BREATH ANALYSIS —

.079 ADJUSTED FOR 29.73 in ✓  
ALCO TARGET .078 16:18  
BLANK TEST .000 16:19  
INTERNAL STANDARD VERIFIED 16:19  
ALCO TV 29.73 in .000 ✓ 16:19  
BLANK TEST .000 16:20  
SUBJECT SAMPLE .000 16:20 C 1/13/10  
BLANK TEST .000 ✓ 16:21  
ALCO TV 29.73 in .000 16:21  
BLANK TEST .000 16:22

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 130193 ✓

JANUARY 06, 2010 ✓  
TIME 16:24

### — DIAGNOSTIC CHECK —

COMPUTER: OKAY  
PROGRAM: OKAY  
SOFTWARE DATE: 01/08/09  
HEATERS  
SAMPLE CHAMBER: 49c  
BREATH TUBE: 41c  
BAROMETER: 29.73 in  
FLOW DETECTOR: OKAY  
PUMP  
HIGH SPEED: OKAY  
DETECTOR: OKAY  
FILTERS: OKAY  
QUARTZ STANDARD: OKAY  
CALIBRATION: OKAY

### PRINTER TEST

!""%&'()\*+,-./0123456789:;<=>?@ABCDEF G  
HIJKLMNPOQRSTUVWXYZ[\]^\_`ab cdefghijklmno  
pqrstuvwxy z{ }~■